



CERTIFICATION by CUSTODIAN of RECORDS

Tucson Police Department Crime Laboratory  
270 S. Stone Avenue Tucson, AZ 85701-1917

I hereby certify that these documents are a true and correct copy of the periodic maintenance\* for the Intoxilyzer 8000 Serial Number 80-001199 maintained by the Tucson Police Department Crime Laboratory pursuant to the requirements of the Arizona Department of Public Safety for a quality assurance program.

A quality assurance specialist (QAS) tested the instrument on the following dates. The acceptable accuracy limits, as defined in A.A.C. R13-10-104.A.2, for a 0.100AC solution are 0.090AC to 0.110AC.

Date: 3-31-11 Cal 1 0.100 AC Cal 2 0.100 AC

Between the dates of 3-3-11 and 3-31-11 the instrument was operating properly and accurately.

The instrument was taken out of service for repair on N/A.  
The instrument was returned to service on N/A.

Clare Conley

Clare L. Conley


3-31-11

ADPS QAS Permit # 33314

SUBSCRIBED AND SWORN to before me this 31, day of March, 20 11.

Laura B. Hodgson

Notary Public

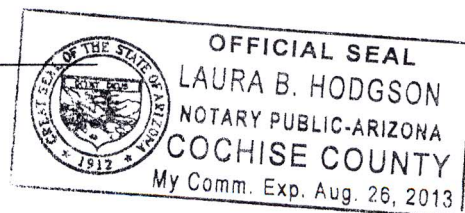

\*Includes documents specified in A.A.C. R13-10-104.A.5

EXHIBIT G-4

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

1-87  
an  
TS4  
3-31-2011

QA SPECIALIST Clare Conley AGENCY Tucson Police Department

DATE 3-31-11 TIME 0831

INTOXILYZER SERIAL # 80-001199 LOCATION ODW Du1 HQ

(✓) 1. Display reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

(✓) 1. Clock time check.

(✓) 2. Date check.

OPERATIONAL TESTS

(✓) 1. Alcohol-free subject test result 0. 000 AC.

(✓) 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed

(✓) 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.

(✓) 4. Standard Calibration Check standard 0. 100 AC  
Result: 0. 100 AC

Instrument is operating properly and accurately. YES ✓ NO       

COMMENTS None.  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE Clare Conley

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-001199  
03/31/2011

08:33:44

Standard Lot#: 719919  
Last Changed By: C. MORAND #24219

QAS: C. CONLEY #34517  
TUCSON PD

Operator: C. CONLEY #34517  
TUCSON PD

Subject: TEST, SQAP  
DOB: 11/11/1111  
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:34:41
Diagnostic Test	Pass	08:35:08
Air Blank	0.000	08:35:35
0.100 Cal Check	0.101	08:35:54
Air Blank	0.000	08:36:24
Subject Test	0.000	08:36:50
Air Blank	ABT*	08:36:57
Air Blank	0.000	08:37:25

\*Sequence Aborted

### Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-001199  
03/31/2011

08:37:53

Standard Lot#: 719919  
Last Changed By: C. MORAND #24219

QAS: C. CONLEY #34517  
TUCSON PD

Operator: C. CONLEY #34517  
TUCSON PD

Subject: TEST, SQAP  
DOB: 11/11/1111  
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI+	08:38:24
Air Blank	IPS**	08:38:49

\*RFI Detect

\*\*Improper Sample

### Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.

INTOXILYZER 8000  
Location: TUCSON POLICE DEPT  
Serial Number : 80-001199  
03/31/2011

08:38:56

4507  
on

TS4

Standard Lot#: 719919  
Last Changed By: C. MORAND #24219

QAS: C. CONLEY #34517  
TUCSON PD

Operator: C. CONLEY #34517  
TUCSON PD

Subject: TEST, SQAP  
DOB: 11/11/1111  
Sex: M Weight: 111

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	08:40:05
Diagnostic Test	Pass	08:40:32
Air Blank	0.000	08:41:00
0.100 Cal Check	0.100	08:41:19
Air Blank	0.000	08:41:48
Subject Test	0.079*	08:44:56
Air Blank	0.000	08:45:28
Air Blank	0.000	08:45:55
Subject Test	XXX**	08:47:15
Air Blank	0.000	08:47:48

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

### Not a Successfully Completed Test Sequence

Pursuant to section 28-1327, Arizona Revised Statutes, this document is a certified duplicate of the information contained in computer storage devices of the Tucson Police Department.



INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-001199

03/31/2011

08:48:03

Standard Lot#: 719919

Last Changed By: C. MORAND #24219

QAS: C. CONLEY #34517

TUCSON PD

134

5367  
Dr

Test	g/210L	Time
Air Blank	0.000	08:48:31
Cal Check	0.100	08:48:49
Air Blank	0.000	08:49:19

Clare Conley  
Operator's Signature

EXHIBIT G-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY  
A.A.C. R13-10-104(A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000  
STANDARD CALIBRATION CHECK PROCEDURE

6-57  
OK  
TS4  
3-31-2011

QA Specialist Clare Conley AGENCY Tucson Police Department  
DATE 3-31-11 TIME 0831  
Intoxilyzer Serial # 80-001199 Location ODW Det HQ

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0. 100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach  $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 100 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Clare Conley

DPS Form Exh G-2 (Rev. 05-01)

INTOXILYZER 8000

Location: TUCSON POLICE DEPT

Serial Number: 80-001199

03/31/2011

08:31:51

-----  
Standard Lot#: 719919

Last Changed By: C. MORAND #24219  
-----

QAS: C. CONLEY #34517

TUCSON PD  
-----

Test	g/210L	Time
Air Blank	0.000	08:32:18
Cal Check	0.100	08:32:37
Air Blank	0.000	08:33:06

*Clare Conley*

\_\_\_\_\_  
Operator's Signature